

PRODUCT DATA SHEET

Stationary

Ultrasonic Flowmeter

UFL-30

TOKYO
KEIKI

TOKYO KEIKI INC.

1. Outline

- 1) Transit times of ultrasonic pulses transmitted in a liquid vary with the flow velocity of the liquid and ultrasonic flowmeters utilize this characteristic to measure flow.
- 2) Regardless of whether the liquid is electrically conductive or non-conductive, ultrasonic flowmeters can measure various types of liquids such as potable water, river water, industrial water, agricultural water, wastewater, seawater, and pure water.
- 3) Transducers are clamped on to the outside of the pipe so it is not necessary to cut pipes or stop flow for installation and there is no pressure loss.
- 4) Flow measurements are possible over a wide range, -30m/s to +30m/s.
- 5) Economical measurements of flow from 25mm to 6000mm can be obtained.
- 6) Easy Operation through PC configuration software. Through graphical user interface, it is very simple and useful for everyone to input all data.



2. Configuration

Flowmeter components

Component	Model	Quantity	Description
1. Main unit	UFL-30	1 pc	Flowmeter main unit
2. Transducers	25mm-250mm Pipe 1MHz Sensor	1 path measurement: 2 pcs 2 paths measurement: 4 pcs 4 paths measurement: 8 pcs(*)	Ultrasonic transmit and receiving transducers and pipe-mounting fixtures for transducer (integrated transducer cable; length: 5m (standard))
	300mm-6000mm Pipe 0.4MHz Sensor		
3. Coaxial cable	5C-2WAE	1 path measurement: 2 pcs 2 paths measurement: 4 pcs 4 paths measurement: 8 pcs(*)	Connection cable between flowmeter main unit and transducers (max. cable length: 300m)
4. Multi-path Junction Box (*)		1 unit	Channel expansion junction box for 4paths measurement

(*) Multi-path measurement and multi-path Cable Junction unit for 4 paths are optional specifications.

1MHz transducer (pipe dia. less than 300mm) components are as follows.

Components		Transducer (single set standard qty)			Material	Weight (appx.)
		1path measurement	2paths measurement (*2)	4paths measurement (*2)		
1. Transducer		1pair (2pcs)	2pair (4pcs)	4pair (8pcs)	Case material SCS13	1.4kg / 2pcs
2. Mounting bracket		1pc	2pcs	4pcs	SUS304	2.9kg / pc
3. Clamp (*1) (SUS belt)	125mm-250mm	3pcs	3pcs	3pcs	SUS304	35g / pc
	25mm -100mm	2pcs	Option (*3)	Option (*3)	t:0.6mm	
4. Cover (*4)		1pc	2pcs	4pcs	SUS304 color: 5Y7/1	0.5kg / pc

SCS and SUS is notation by Japanese Industrial Standard for kind of stainless steel material.

(*1) 125mm ~ 250mm: pipe dia. (more than 125mm, less than 250mm)
25mm ~ 100mm: pipe dia. (more than 25mm, less than 100mm)

(*2) 2 or 4 paths measurement is optional specifications

(*3) Multiple paths measurement for pipe diameter less than 100A is required application specific mounting fixture. Consult Manufacturer.

(*4) Cover, optional specifications

0.4MHz transducer (pipe diameter more than 300mm) components are as follows.

Components		Transducer (single set standard qty)			Material	Weight (appx.)
		1path measurement	2paths measurement (*1)	4paths measurement (*1)		
1. Transducer		1pair (2pcs)	2pair (4pcs)	4 pair (8pcs)	Case material SCS13	2.0kg / 2pcs
2. Mounting bracket		2pcs	4pcs	8pcs	SUS304	1.9kg / 2pcs
3. Tightening fixture	Less than 1600mm	2pcs	2pcs	2pcs	SUS304	5.2kg / 2pcs
	More than 1600mm	4pcs	4pcs	4pcs		
4. Wire rope	Less than 1600mm	4pcs	4pcs	4pcs	Stainless	180g / 1m
	More than 1600mm	8pcs	8pcs	8pcs		
5. Transducer cover (*2)		2pcs	4pcs	8pcs	SUS304 Color: 5Y7/1	0.7kg / 2pcs

SCS and SUS is notation by Japanese Industrial Standard for kind of stainless steel material.

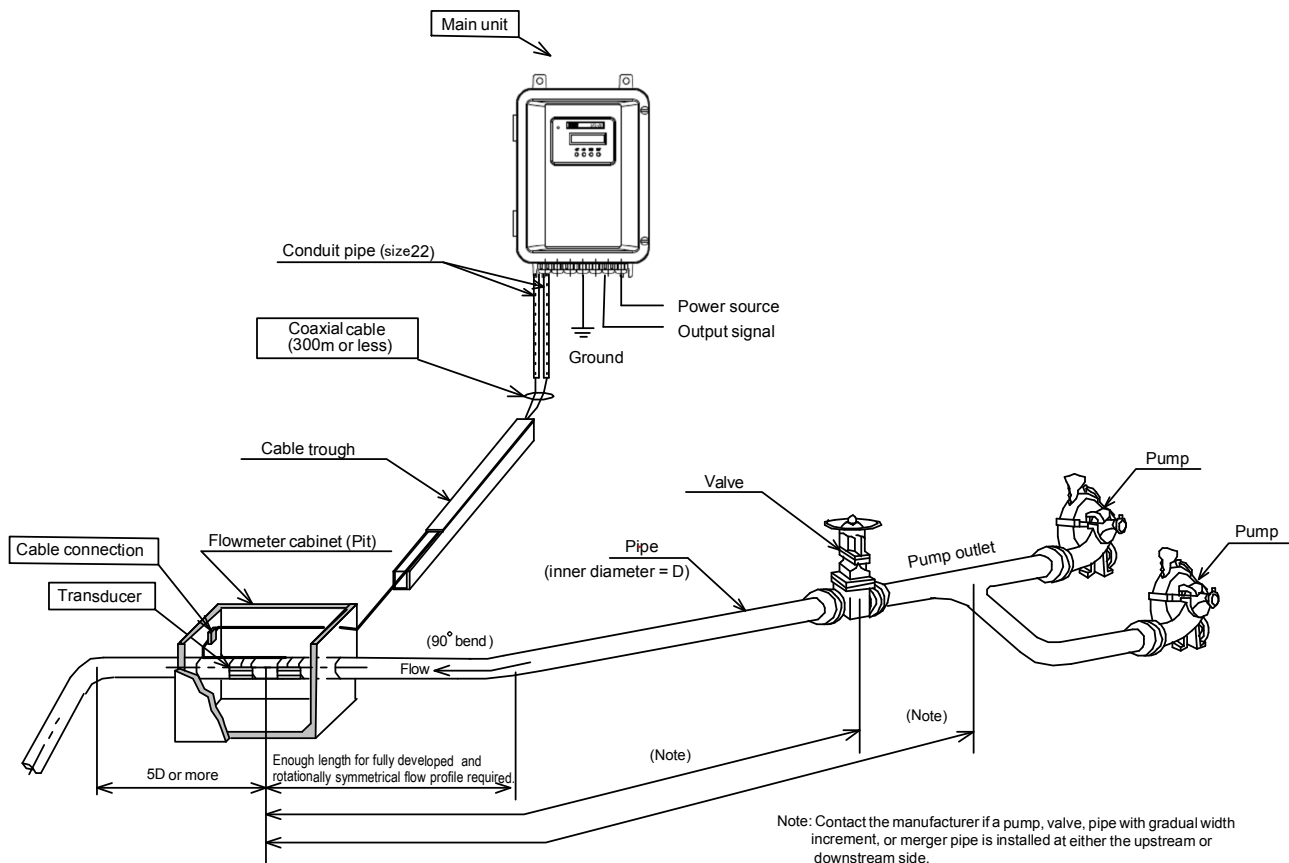
(*1) 2 or 4 paths measurement is optional specifications.

(*2) Transducer cover is optional specifications.

3. Specifications

3-1. Overall Specifications

Measurement	Fluids	Homogeneous and sonically conductive fluids (water, waste water, industrial water, river water, sea water, pure water, etc.)
	Temperature range	-20°C to +115°C (depend on transducer) Note: 1) above also applicable to ambient temperature 2) For main unit, -10°C to +60°C
	Turbidity	10000 mg/L or less
Pipes	Material	Materials which allow stable transit of ultrasonic waves such as steel, SUS, castings, ductile casting, PVC, FRPM, etc. Note: Applicable diameters may vary with material.)
	Diameters	DN25mm to DN6000mm
	Lining	None, tar epoxy, mortar, etc.
Measurement Range	Converted to flow velocity: -30 m/s to +30 m/s	
Measurement Cycle	60 ms	
Measurement Accuracy	D ≥ 300mm, ±1% of reading, however ±0.008m/s for velocities less than 0.8m/s. D < 300mm, ±1% of reading, however ±0.02m/s for velocities less than 2m/s. Note: 1) For volumetric flow rate. 2) Fully developed and rotationally symmetrical flow profile required.	
Repeatability	±0.5%	
Range ability	1 : 300	
Measurement Method	Ultrasonic pulse transit time difference method	



3-2. Main Unit

Analog output	St'd/option	Standard
	Output	Instantaneous flow rate Number of outputs: 2 Output pattern: 1 system parallel output, 8 types 2 system output, 10 types Special output, 1 type Note: 1) Instantaneous flow rate will change to velocity value in case of velocity mode. 2) Ch2 output will be the same type as ch1 output when 1 system or special output is selected. (parallel output)
	Output format	4 - 20mA (1 system / 2 system output) 0.8 - 20mA (special output) 20.8mA (Burnout when no echo received or during failure warning (span +5%) output possible) Max. allowable load resistance 1 K ohm, insulated outputs
	Terminal panel	Screw less Terminal (0.08~2.5mm ² cable applicable)

Contact point output	St'd/option	Standard
	Output	For each of the 4 contact points, output selection allocation as follows. (parallel output possible) 1. Forward flow totalized pulse 2. Backward flow totalized pulse 3. No echo received warning 4. Equipment failure warning 5. Equipment failure or no echo received warning 6. Upper limit warning 7. Lower limit warning 8. Forward flow detection 9. Backward flow detection 10. High range detection 11. Low range detection 12. Not used Note: 1) Pulse width of contact is selectable from 1000,500,100 or 20ms. But not for both forward and backward. 2) Each default setting is "ON" at work, but "OFF at work is also selectable.
	Output format	Photo coupler (insulated)
	Contact point capacity	DC48V, 0.4A
	Notes	Totalize units 0.01L, 0.1L, 1L, 10L, 100L, 1m ³ , 5m ³ , 10m ³ , 100m ³ , 1000m ³ , 10000m ³ 1g, 10g, 100g, 1kg, 10kg, 100kg, 1t, 10t, 100t, 1kt, 10kt, 100kt ft ³ ,kft ³ ,Mft ³ , bbl, kbbl, Mbbl, gal, kgal, Mgal, acf, kacf, Macf Valid units may be limited depending upon the selected flow unit.
	Terminal panel	Screw less Terminal (0.08~2.5mm ² cable applicable)

Digital output	St'd/option	Standard
	Output 1	<p>One-way output mode</p> <p>Following data is output per set output cycle Instantaneous flow rate, forward/backward flow totalized value and various warnings. (flow meter mode: linear flow rate and various warnings)</p> <p>Note: Instantaneous flow rate will change to velocity value in case of velocity mode. No totalized values available.</p>
	Output 2	<p>Intercommunication mode</p> <p>Connection to PC enables setting of flowmeter unit, setting menu and reading of measurement values and operation status.</p>
	Output type	RS232C (non-insulated output)
	Output cycle	1 to 3600 seconds possible (output 1 only)
	Communication speed	4800 bps, 9600 bps or 19200 bps selectable
	Data bit length	8 bit/1 stop bit
	Parity check	EVEN
	Format	Original Format (ASCII) MODBUS (Selectable; only for Output1)
	Synchronization	Asynchronous
	Cable length	Up to 3m
		Note: To comply with EC directives, use less than 3m cable.

Multi-path measurement	St'd/option	Option
	Quantity	2 path or 4 path
	Details	<p>2 path:</p> <ul style="list-style-type: none"> - 1 additional pulser module required and installed in main unit (total 2 modules). - Transducer, fixture, extension cable for each path required. <p>4 path:</p> <ul style="list-style-type: none"> - External multi-path junction box is required and 2 special coaxial composite cables are connected to the flowmeter main unit. - Transducer cable connected in junction box by BNC connector. - 3 additional pulser modules required and installed in main unit. (Total 4 modules). - Transducer, fixture, extension cable for each path required.

Data setting	Setting method	PC connected to Digital Output port 2, setting through PC with configuration software (LCD 4-keys entry is available, but limited).
	Setting items	Indication, Unit (Flow rate and Totalizing) Flow Range and various settings

Measurement display	Display method	LCD (16 character x 2 lines), with backlight Over 5 years life (by 25°C)							
	Display content	Switchable display of following: <ul style="list-style-type: none"> • Instantaneous flow rate, warnings, check mode and totalizing status. • Instantaneous flow velocity value, warnings check mode and totalizing status. • Forward flow totalized value, warnings, check mode and totalizing status. • Backward flow totalized value, warnings, check mode and totalized status. • Status1 (AGC, Range, Warnings and Check mode) • Status2 (Number of R-OFF warning & Disturbance Elimination function worked.) <p>Note:</p> <ol style="list-style-type: none"> 1) During power failure, displayed screen component is memorized and displayed when power is again introduced. 2) Instantaneous flow velocity of each path can be indicated on display in case of multi-path installation. 3) Counter can be reset by key pad operation. 							
	Display digits	Instantaneous flow rate:	Dependent on max. flow rate for Analog output setting. Max. 7 digits including sign, decimal point. <table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <td style="width: 30%;">Forward</td> <td style="width: 30%;">Max. 7 digits Including Decimal point</td> <td style="width: 40%;">Range: 0 to 99999.0</td> </tr> <tr> <td>Backward</td> <td>Max. 7 digits including Sign and Decimal point</td> <td>Range: -0 to -99999</td> </tr> </table>		Forward	Max. 7 digits Including Decimal point	Range: 0 to 99999.0	Backward	Max. 7 digits including Sign and Decimal point
Forward	Max. 7 digits Including Decimal point	Range: 0 to 99999.0							
Backward	Max. 7 digits including Sign and Decimal point	Range: -0 to -99999							
	Instantaneous flow velocity:	sign section	1 digit						
		integer section	2 digits						
		decimal fraction	3 digits fixed						
	Totalized flow:	7 digits							
	During exceeding Max. range of flow rate for Analog output setting, indication would be "Instantaneous flow rate" and alternated flickering with "FS" (Full Scale) mark.								

Measurement display	Display content	
(cont.)	Warnings	Backup battery remaining life - "B" displayed when battery voltage falls below prescribed value. Not detectable when battery would not be equipped itself.
		No Echo received warning - "R" displayed during processing when no wave received.
		Disturbance Detection - "D" displayed when the measuring condition disturbed by air bubbles, solids or other factors.
		Over Range - "O" displayed when the measuring value exceeds upper or lower limitation setting.
		Check
	Totalizing Status	"I" displayed blinking when totalizing function operated.
	Failure warning	"ERR01" to "ERR63" displayed during equipment failure. Check operation display is replaced by this failure display.
	Status 1	"AGC" displayed in case of AGC function on.
		"LO-RNG" displayed in case of low range output.
	Status 2	"HI-RNG" displayed in case of high range output.
Number of "R-OFF warning" function worked. Number of "Disturbance Elimination" function worked.		

Function	Low flow cut	Cuts (zeros) flows when flow falls below prescribed instantaneous flow rate. Used in order to avoid output of flow values other than 0 when measurement value during still flow becomes disordered.
	No Echo receiving warning	<p>If measurement cannot be made when no echo is received continuously over the setting time (determined transition time), status is changed to</p> <ul style="list-style-type: none"> - Selected analog output type Selectable analog output transition status as follows. 0% (4mA), hold, 100% (20mA), burnout (20.8mA) - Display "R" on LCD. - Contact output of warning if set. <p>Note:</p> <ol style="list-style-type: none"> 1) Measurement values and analog output will be restored when echo is received continuously over the setting time (determined restore time). 2) In case of multi-paths, processing can be selected to change output for no echo receiving for 1 path or for all paths. Initial setting value is for no echo receiving for all paths. 3) If measurement can be made for even 1 path, measurement will be continued for only this path.
	Disturbance detection	<p>Check whether processing values are measured properly or not and if determined to be disturbed conditions then measuring values are eliminated.</p> <ul style="list-style-type: none"> - Display "D" on the display - Count up as history on status 2
	Zero Shift compensation	Zero point can be independently compensated (shifted) for forward and backward flow rate.
	Span compensation	Slope of span line can be independently compensated for forward and backward flow rate in the range 0.100 to 2.000.
	Filtering (Smoothing)	<p>Rapid flow rate changes would be smoother by this filter for 1 to 120 sec. (Default 15sec)</p> <p>Note: This value is meaning the time until measuring flow rate reaches 90% by step-up increment.</p>
	Self-diagnostics and failure processing	<p>Self-diagnostics is run periodically.</p> <p>If failure is diagnosed on following items, transitions to be selected status.</p> <p>Diagnostic checks:</p> <ol style="list-style-type: none"> 1) Memory Area check (for totalizing and setting parameter) 2) Parameter check 3) Time measurement counter malfunction 4) Transmitter malfunction 5) Receiver malfunction <ul style="list-style-type: none"> - Selected analog output transition status as follows. 0% (4mA), hold, 100% (20mA), burnout (20.8mA) - Display "ERR**" on LCD. (** is error number.) - Contact output of warning if set. <p>Note: "AND" , "OR" condition is selectable in accordance with fault tolerance function setting.</p>

Function (cont.)	Data retention	Totalized flow values and all setting parameters are retained in memory with lithium battery even if power failure. Note: 1) Setting Parameters are retained in nonvolatile memory. 2) Totalized flow value and ROFF/Disturbance detection history are retained in memory which hold by Back-up Battery. 3) Data retained in memory which hold by Back-up Battery clears if battery removed without power supply. 4) 5 year life at room temperature. 5) No battery recharging function.
	Analog output check	Output can be freely changed depending on analog output setting. Setting every 0.1% of flow span range (-120.0 to + 120.0) possible.
	Path fixing	Measurement of specified path can be fixed and flow checked for every path when using multi-paths.
	Automatic Gain adjustment (AGA Function)	Receiver gain can be set as ideal amplitude by automatically or manually. (Manual gain setting is done conventionally by monitoring receiving echo with oscilloscope)
	Analog output range switching	Analog output range is automatically switchable when double range mode.
	Automatic gain control (AGC Function)	Receiver gain is automatically adjusted to the optimum level in response to changes in receiver sensitivity during measurement. Note: Not available in case of containing air bubble or nearby flow control valve.
	Forward / Backward flow change processing	Hysteresis can be set by time in order to avoid flapping of direction detection contact points when there are back and forth, plus and minus changes in measurement values during still water condition.
	Totalized value preset	Totalized values can be freely preset. Preset Range: 0 to 9999999
	Basic data display	Following internal data can be referenced. - Fluid sonic velocity (unit, m/s) - Reynolds Number - Amp. Gain
	Error historic counter	Count "No Echo receiving warning" & "Disturbance detection" when it occurred.

Power supply	AC100 to 230V +/-10% (50/60 Hz±10%) Option : DC24V±20% (This option must be pre-selected)
	Momentary outage AC input: 20ms, DC input: 5ms
Power consumption	AC100V: 20VA / AC200V: 27VA DC24V: 10W (Option)
Fuse	<u>IEC 60127-2 SS5</u> Cartridge fuse-links φ 5.2x20 mm Rating 2A/250V Time-lag High Breaking Capacity (1500A)
Rush Current	Less than 20A at AC100V / Less than 32A at AC200V Less than 30A at DC24V (Option)
Operating temperature range	-10 to +60°C (for main unit ambient)
Storage temperature range	-20 to +70°C
Operating humidity range	Less than 90% RH, non-condensation
Main unit construction	Protection Degree IP65 (IEC 60529)
Wiring connection port	Cable gland, 7 pcs, O.D.6~12mm cable applicable
Case material	Aluminum
Coating	Melamine
Color	Munsel 10YR9.4/0.5
Weight	Approx. 8kg
Dimensions	260mm x 394mm x 155mm

European Compliance (CE marking)	EMC Directive 2004/108/EC Harmonized Standard / EN61326-1:2006 Separation into group / Group I Division into classes / Class A Location intended for use / In industrial locations
	Low Voltage Directive 2006/95/EC Harmonized Standard / EN61010-1:2001 Over voltage category II Pollution degree II Altitude up to 3000m

3-3. Transducers

Transducers	Large diameter	SE044040NC	(-20°C to + 65°C)
	Large diameter narrow space	SE042140NC	(-20°C to + 65°C)
	Large diameter high temperature	SE044040N-HT	(+60°C to +115°C)
	Small diameter	SE104720	(-20°C to + 60°C)
	Small diameter high temperature	SE104020N-HT	(+60°C to +115°C)
Note	Water proof performance	Protection Degree IP67 (IEC 60529)	
	Construction	One piece construction with 5m cable	
	Cable	Coaxial cable with double shielded insulation between sheaths	
	Cable max. length	300m	

3-4. Accessories

Cable Junction box	St'd/option	Option
	Construction	IEC 60529 Protection Degree IPX4
	Material	Aluminum casting
	Connection port	4 locations (2 locations each side)
Multi-Path Junction box	St'd/option	Option
	Construction	IEC 60529 Protection Degree IP66
	Material	Aluminum casting
	Connection port	10 locations (2 for Main Unit side & 8 for Transducers side)
	Cables	Included 1m Special Composite Coaxial Cable with Connector to Main unit.
Power Cable (*1)	St'd/option	Prepared by User
	Model name	OLFLEX Classic 100 multi-conductor, flexible power and control cable
	Part Number	10060
	Manufacturer	LAPP KABEL
	Details	3 Conductors AWG16, 1.5 mm ² Nominal Outer diameter 8.1 mm

(*1) Power cable is specified to comply with EC directive.

4. Analog output profiles

Table1: Analog Output Profile Table

(1) Single System Output 1/2





Profile Description		CH1,CH2 Common Output
One-Way Single Range		
Two-Way Single Range		
One-Way Double Range	Automatic Double Range	

(2) Single System Output 2/2





Profile Description		CH1,CH2 Common Output
Two-Way Double Range	Automatic Double Range	
Special		

Table 1 (continued)

(3) Dual System Output 1/2

Profile Description		CH1 Output	CH2 Output
	Two-Way Single Range		
One-Way Double Range Internal Switching	Automatic Double Range		












(4) Dual System 2/2

Profile Description		CH1 Output	CH2 Output
Two-Way Double Range Internal Switching	Automatic Double Range FW/BW		
	Automatic Double Range HI/LO		

5. Transducer installation


- To minimize measurement errors arising from flow profile, a straight pipe run is necessary for transducer installation.
- Liquid should fill the pipes completely and transducers should be installed in locations which have no air bubbles.
- For measurements in underground piping, the usual means is to locate the flowmeter in a pit to facilitate transducer installation, maintenance, and testing.

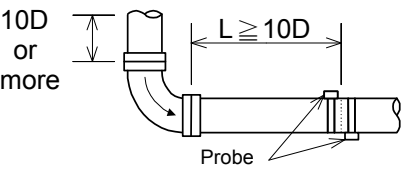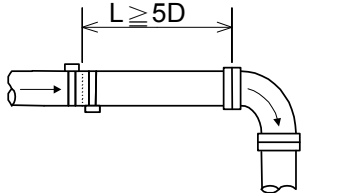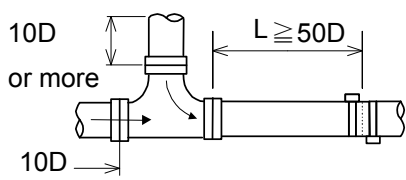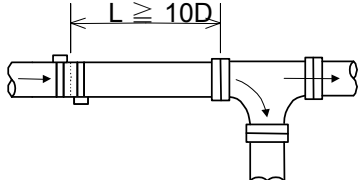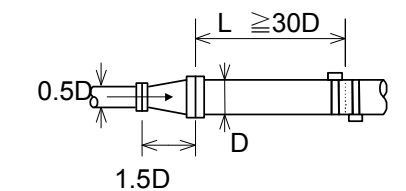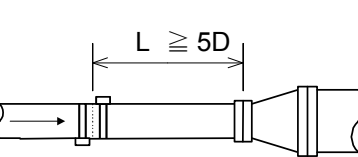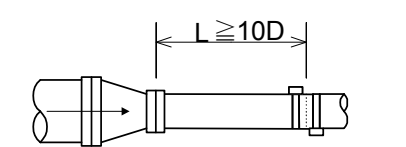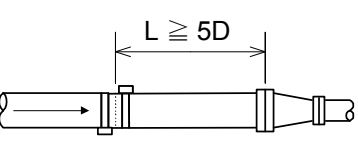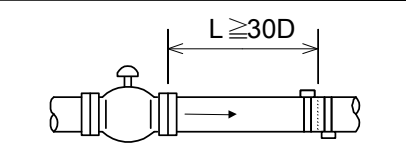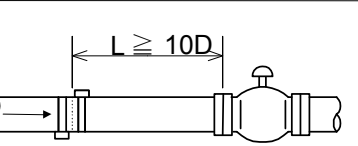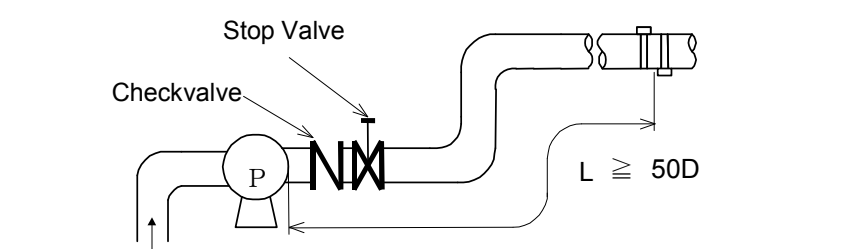[Refer to JEMIS 032-1987]


Structural condition	Upstream straight pipe length	Downstream straight pipe length
90° bend	 <p>10D or more</p> <p>$L \geq 10D$</p> <p>Probe</p>	 <p>$L \geq 5D$</p>
T shape joint	 <p>10D or more</p> <p>$L \geq 50D$</p> <p>10D</p> <p>D</p>	 <p>$L \geq 10D$</p>
Increasing Diameter	 <p>$L \geq 30D$</p> <p>0.5D</p> <p>D</p> <p>1.5D</p>	 <p>$L \geq 5D$</p>
Reducing Diameter	 <p>$L \geq 10D$</p>	 <p>$L \geq 5D$</p>
Control Valves	 <p>$L \geq 30D$</p> <p>Flow Control at upper side</p>	 <p>$L \geq 10D$</p> <p>Flow Control at lower side</p>
Pump	 <p>Stop Valve</p> <p>Checkvalve</p> <p>P</p> <p>$L \geq 50D$</p>	

D : Pipe Diameter

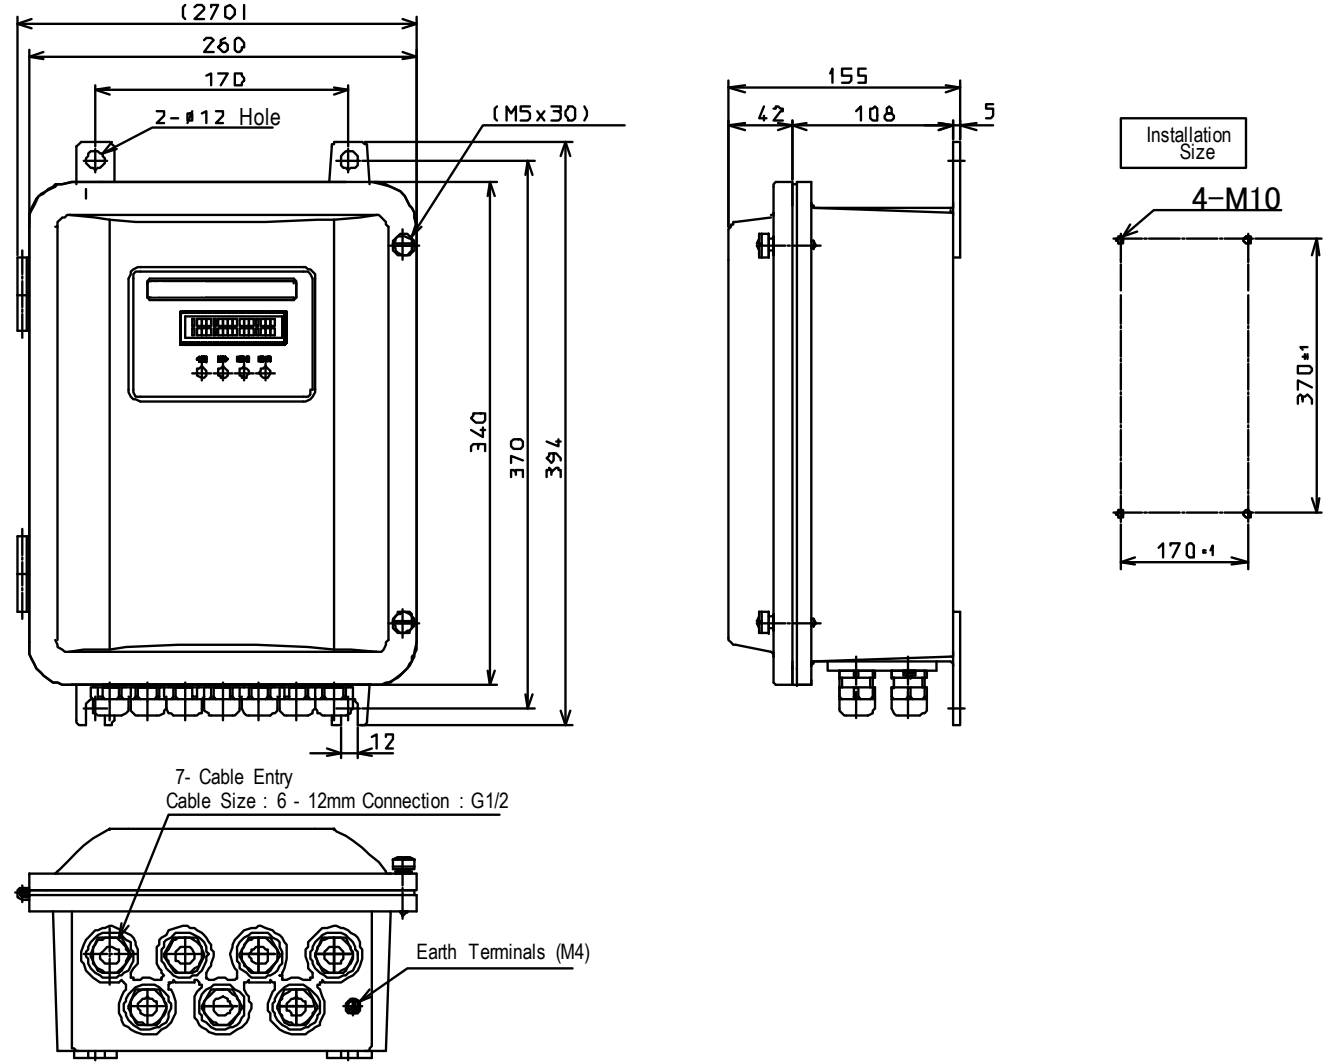
6. Dimensions




Main Unit Dimension

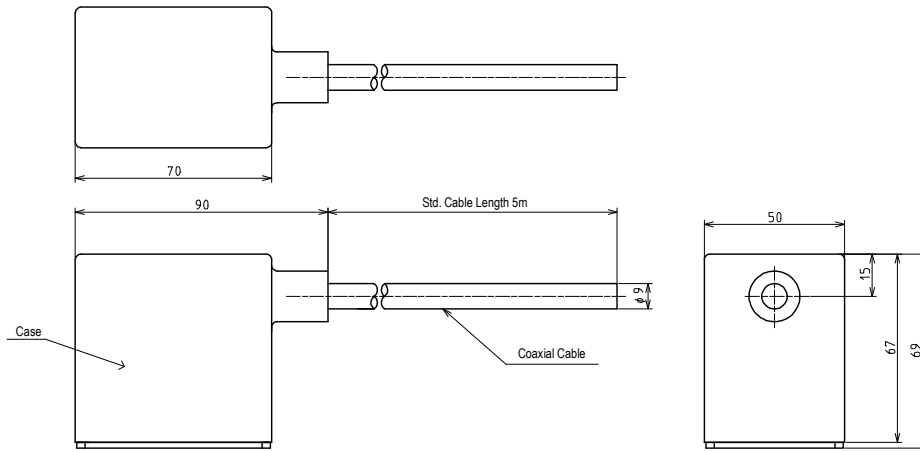

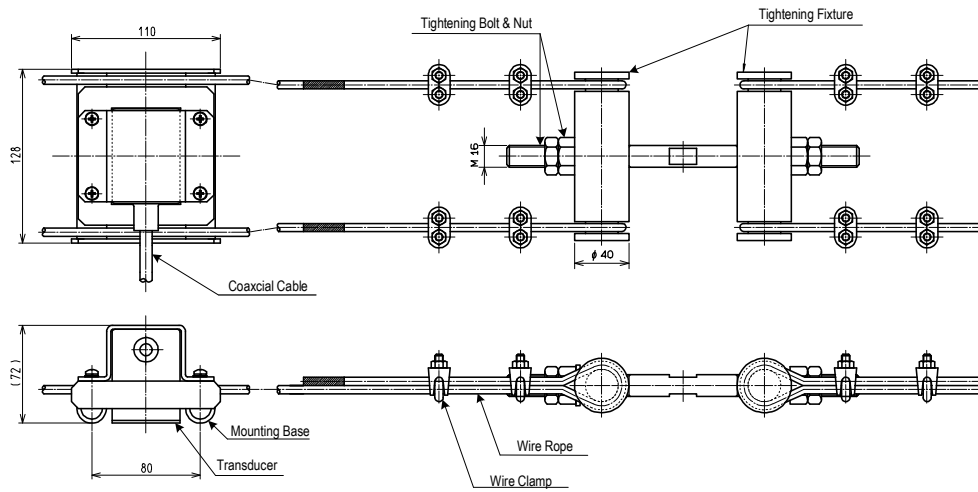
Transducer Dimensions (Pipe Dia more than 300mm)




Mounting Fixture for Transducers

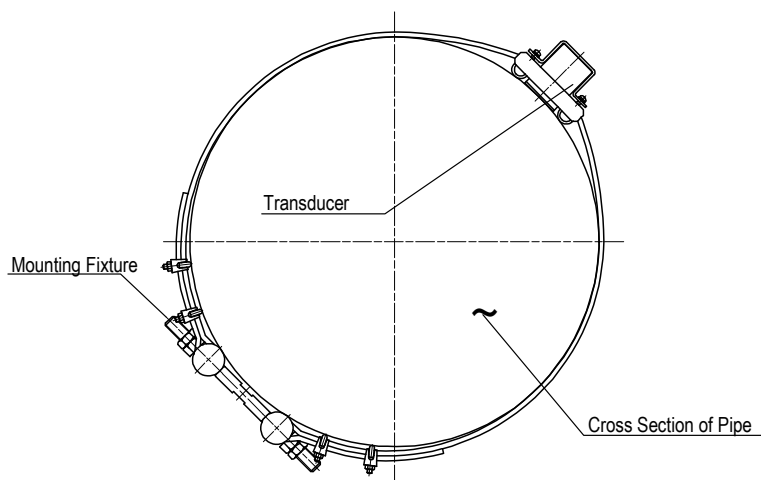


Mounting Example

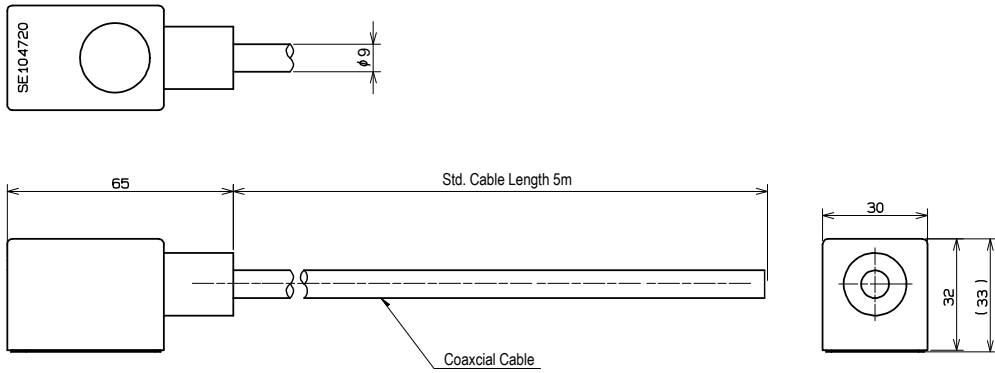

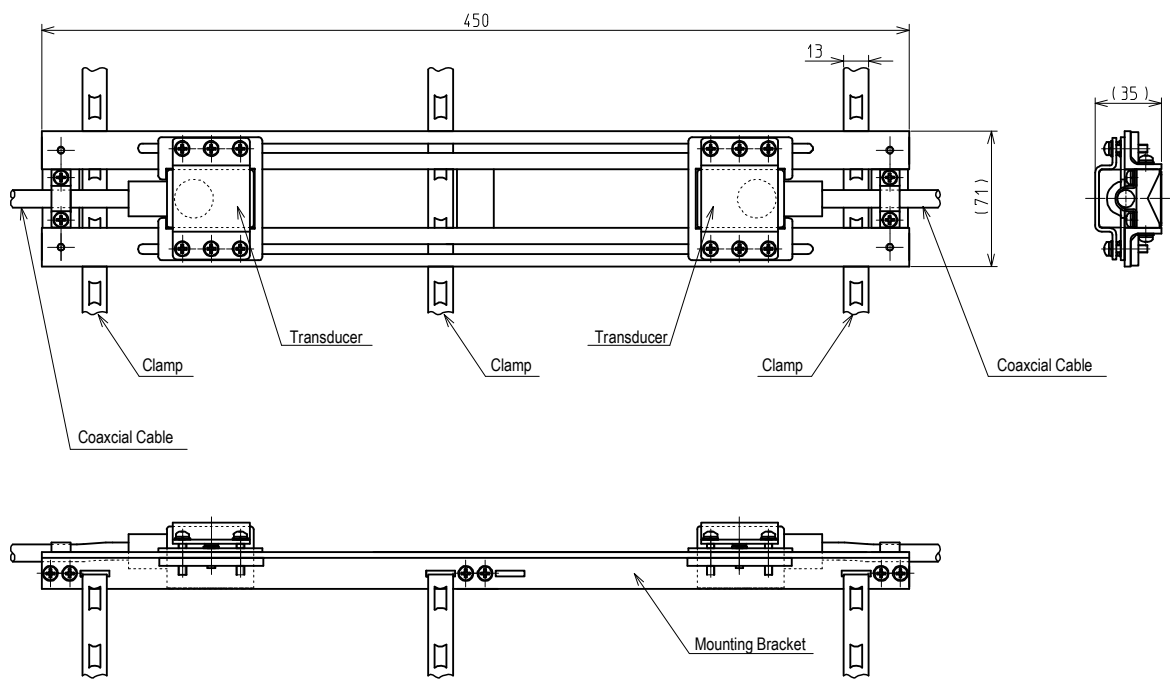Transducer Dimensions (Pipe Dia less than 300mm)




Mounting Fixture for Transducers

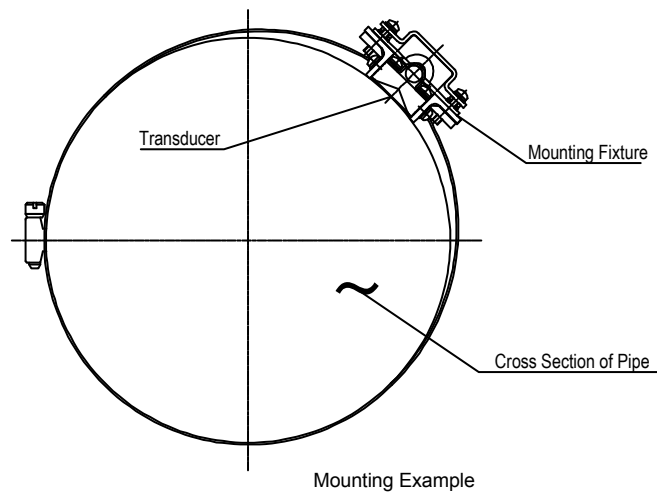


7. Wiring Connection

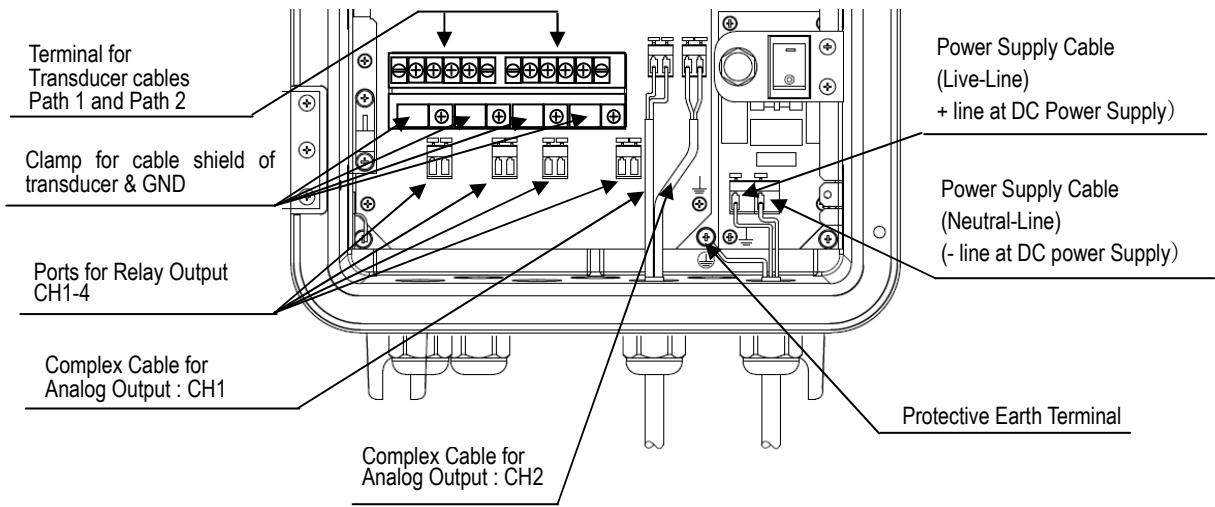
7-1. Output connection




7-2. Cable entry port

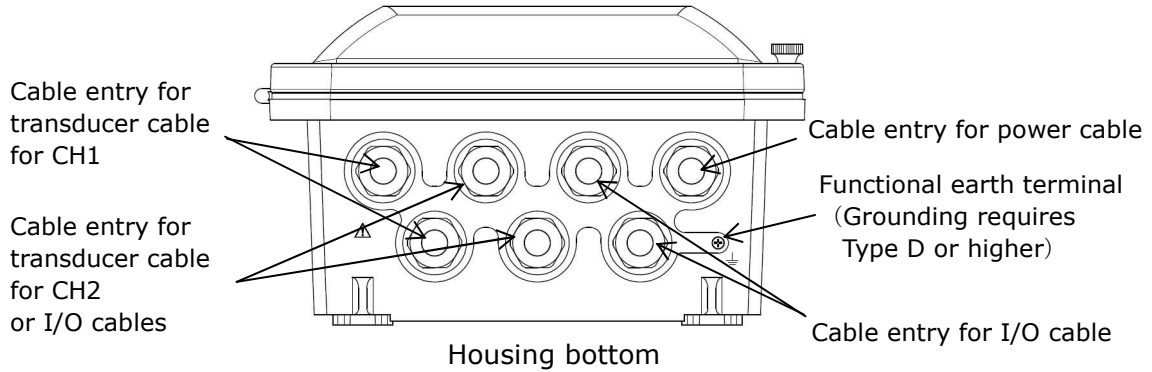

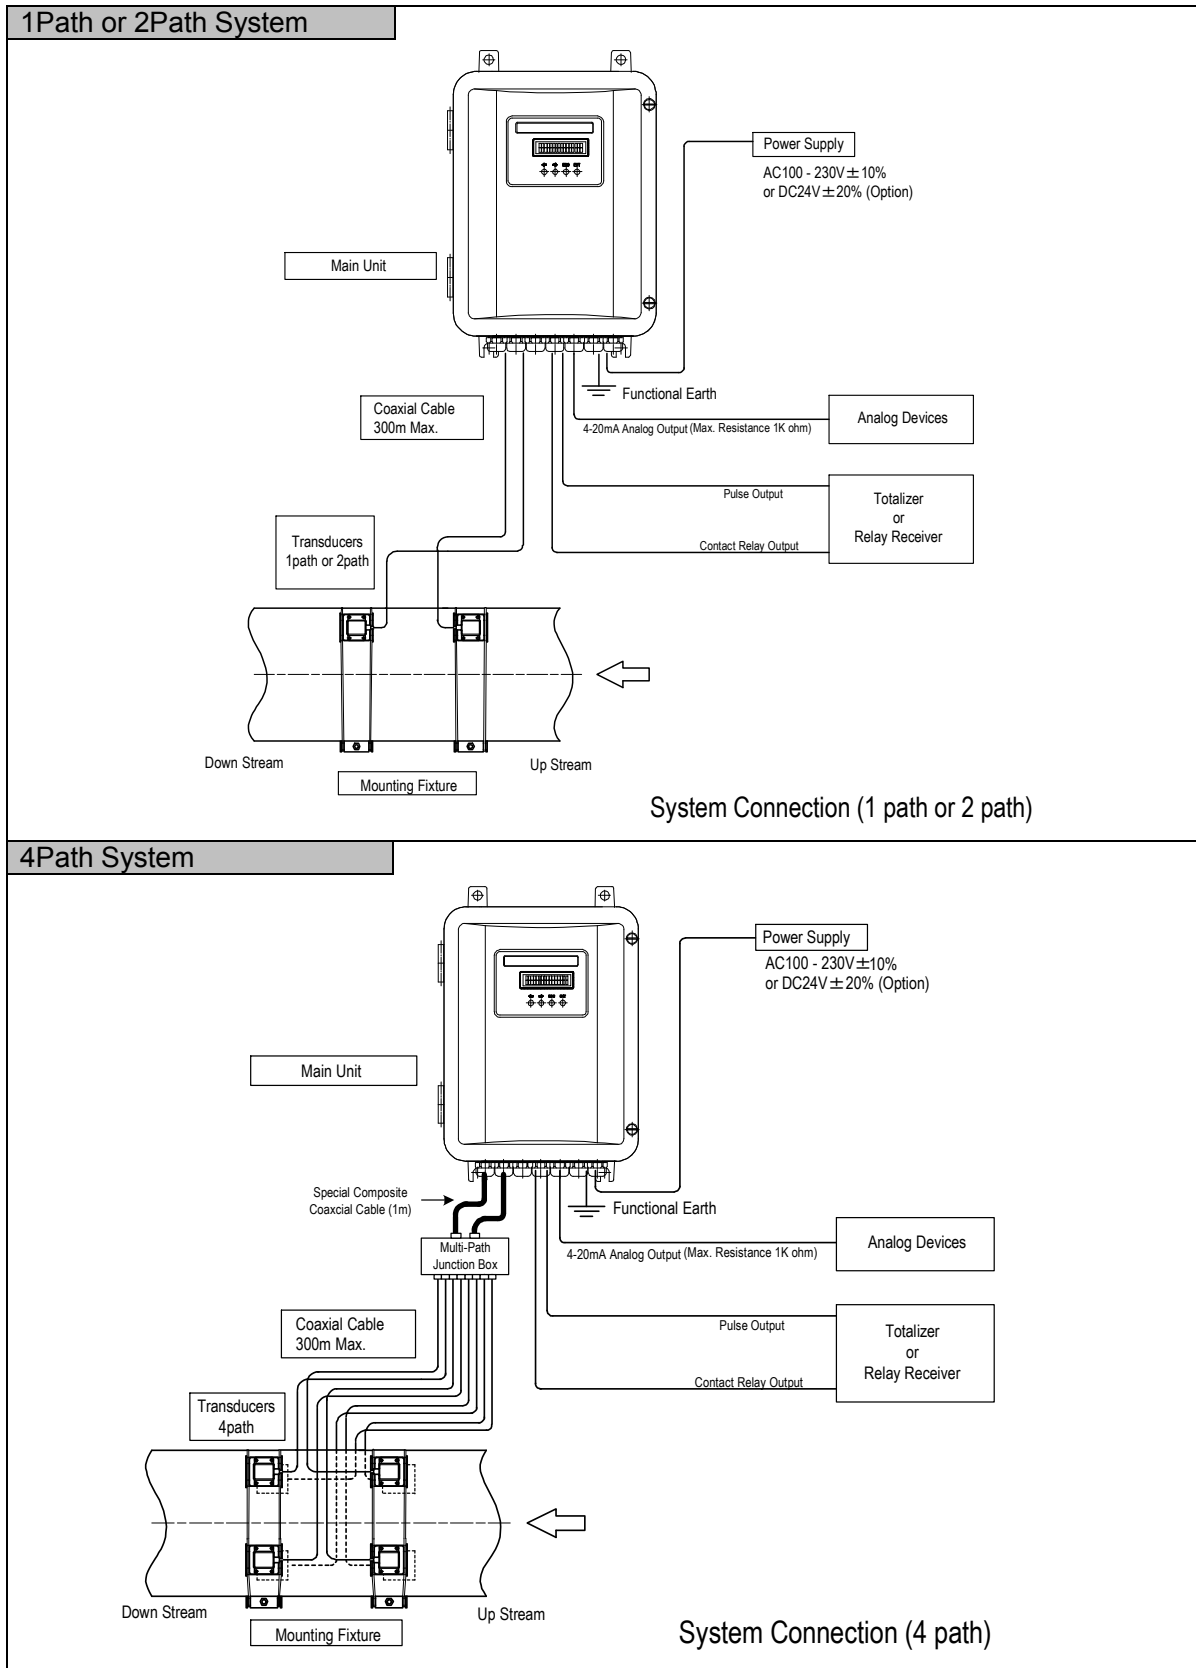8. System Wiring Connection



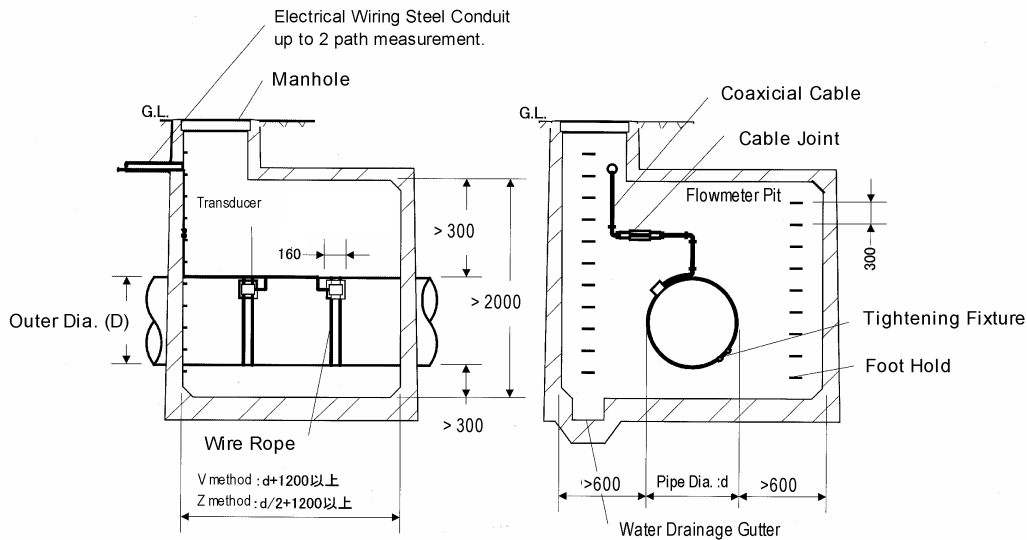9. Building a flowmeter pit



- In principle, when measurement is of underground pipe, it is suggestive to prepare of dedicated flowmeter pit.
- It is not necessary to prepare a flowmeter pit in the case of indoor or outdoor piping, but proper footing should be planned for transducer mounting and equipment adjustments in the case the pipe is located high off the floor or when pipe diameter is large.

Building a flowmeter pit

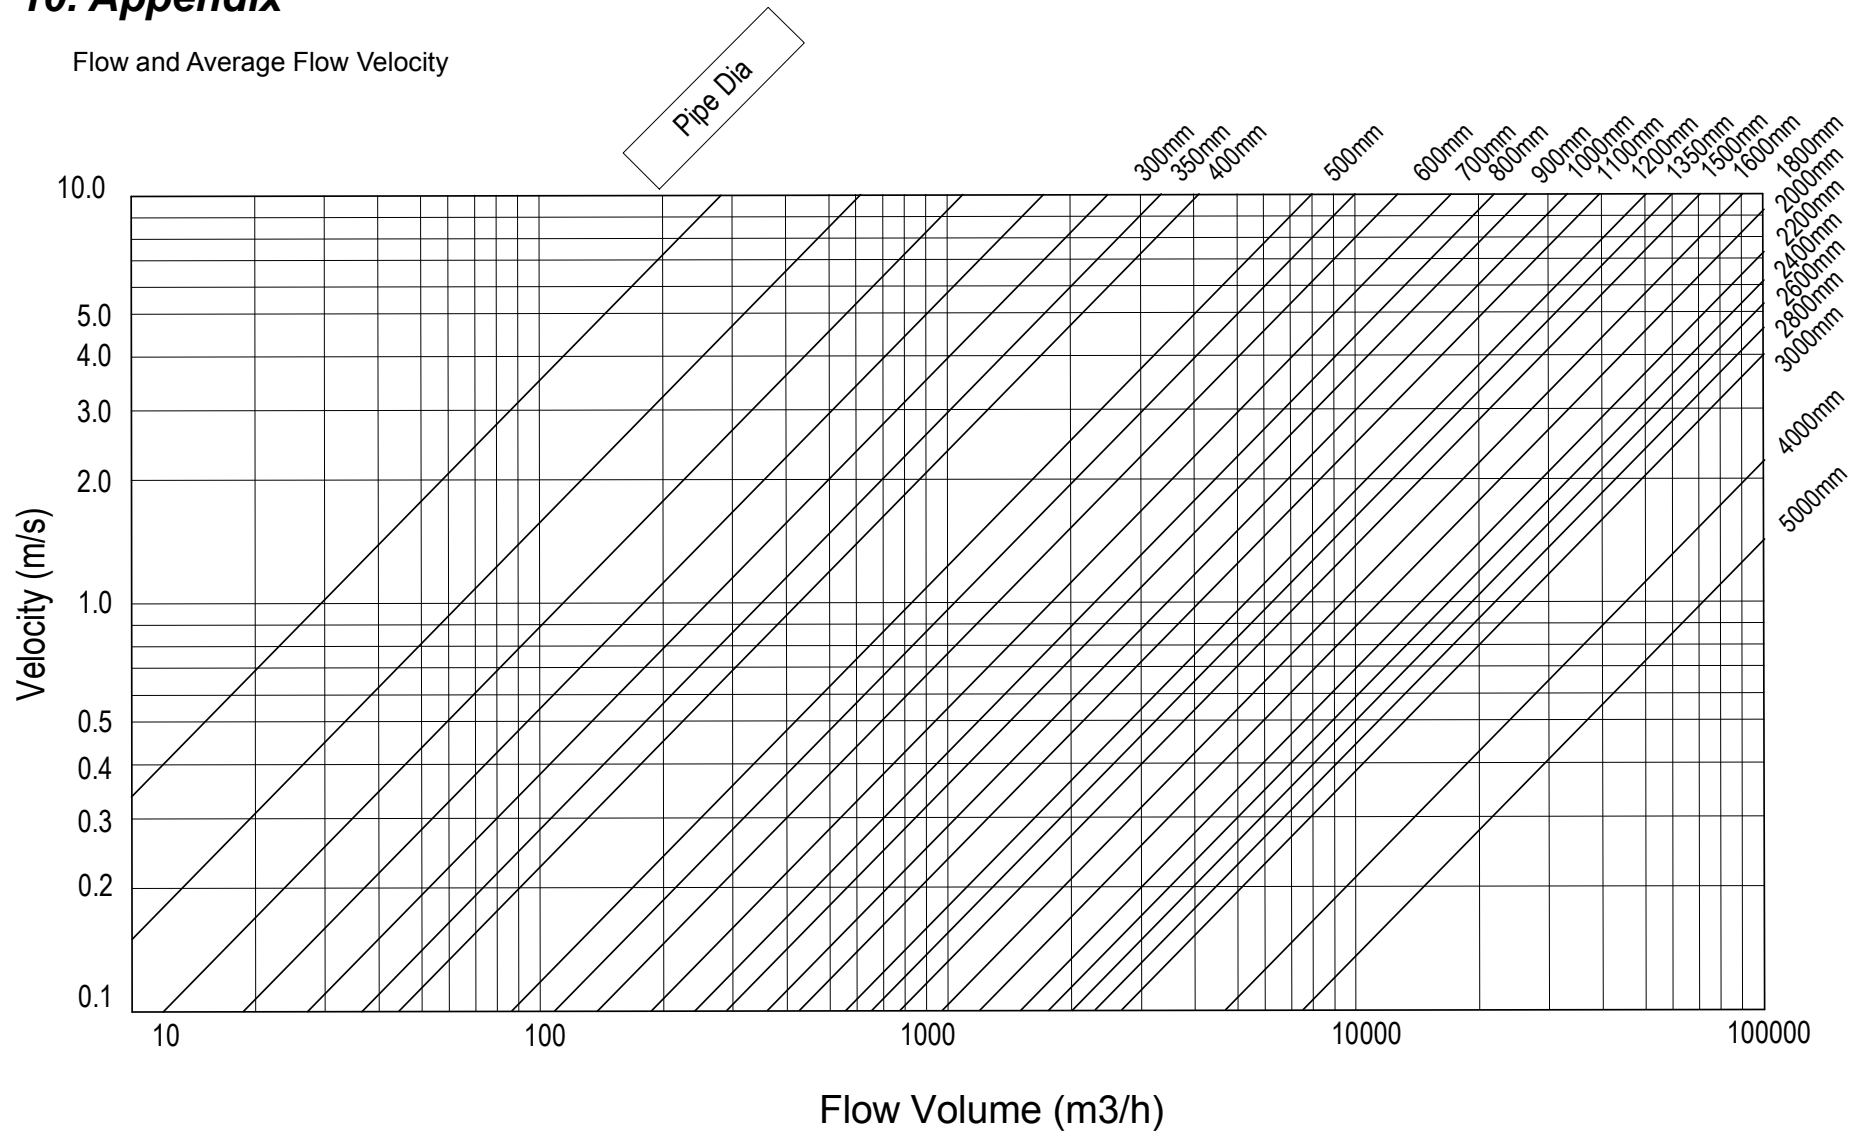
1. Select pit site (taking into consideration the following points)
 - 1) Straight section of pipe is required for installation of transducers as explained under Part 5.
 - 2) Consult manufacturer if an adjustable valve or pump is used.
 - 3) To prevent noise interference or signal attenuation, coaxial cable used between joining material and main unit should be less than 300m.
2. Size and construction of flowmeter pit
 - 1) Using above schematic as reference, determine size of flowmeter pit based on actual piping position and conditions. Height of pit should allow person to stand while working. In cases of pipe diameters greater than 800mm, prepare footholds or footing space.
 - 2) Implement countermeasures for floods such as drainage gutters, etc. (Install water pump where water is liable to accumulate or flood.)
 - 3) Consult Manufacturer for other specific conditions. (Above dimensions are ideal and not the minimum required.)

Transducer installation

1. Strip paint/coating from piping surfaces at transducer mounting locations and fix transducers on piping using the accessory mounting fixtures. When mounting transducers according to the "V" method, the distance separating the transducers should be about the diameter of the pipe. If the "Z" method is used, the distance should be one half of the diameter.
2. After installing and adjusting the transducers, remove transducer mountings, and coat pipe surface with anti-rust paint.

10. Appendix

Flow and Average Flow Velocity



Ultrasonic Flowmeter model UFL-30 Ordering Code List

UFL-30-

--	--	--	--	--	--	--	--	--	--	--	--

 -

--	--	--	--	--	--	--	--	--	--

Component Code
Site Condition Code

Site Condition Code

--	--	--	--	--	--	--	--

Pipe Material	
1	Steel
2	Ductile Iron
3	Stainless Steel
4	PVC
X	Other Material ()

@	Outside Diameter									mm / inch
@	Pipe Thickness									mm / inch

Please fill in forms with actual data.

Lining Material	
1	Tar Epoxy
2	Mortar
X	Other Material ()

@	Lining Thickness									mm / inch
---	------------------	--	--	--	--	--	--	--	--	-----------

Please fill in forms with actual data.

Measuring Liquid	
1	Drinking Water, Raw Water
2	Sea Water
3	Sewage Water (after Screening)
4	Lubricant (Oil)
5	Chiller Water, Heated Water
X	Other Liquid ()

Contact Output (Up to 4 simultaneous outputs)	
1	Forward Totalizing Pulse
2	Backward Totalizing Pulse
3	Receiving Echo Error Alarm (ROFF)
4	Break Down (Unit Failure) Alarming
5	ROFF [or] Break Down
6	High Limit Alarm
7	Low Limit Alarm
8	Forward Direction
9	Backward Direction
A	High Range
B	Low Range
C	BREAK (Normal Open)
D	MAKE (Normal Close)
N	Not Use

Qmax. (Maximum Flow Rate)	
@	

Please fill in forms with actual data.

Please show flow rate's unit also. (ex. m³/h)

This value is related to the setting of maximum range of Analog Output & Indicate-able digits on LCD.

TOKYO KEIKI INC.

2-16-46, Minami-kamata, Ohta-ku,

Tokyo 144-8551

Japan

Control Division I

Fluid Management Systems SBU

Phone : +81-(0)3-3737-8664

Fax : +81-(0)3-3737-8665